Because we care.

MIDMARK®

Installation Instructions

9A305001 ECG Printer Shelf

KIT COMPONENTS

Part Number	Description	Qty
9A305001	Shelf Assembly	1
• 063-9951-00	Shelf, ECG Printer	1
• 040-0250-48	1/4-20 x 1/2 Phillips Screws	2
• 053-0131-11	Velcro, Loop (2"x4")	1
• 053-0105-14	Velcro, Hook (2"x4")	1
• 003-1175-00	Installation Instructions	1

REQUIRED TOOLS

Phillips Screwdriver
Measuring Tape

INTRODUCTION

Provides a location to set a printer on ECG Cart.

CE REPRESENTATIVE

EEC countries should direct all questions, incidents, and complaints to Midmark authorized CE representative: CE

Promotal
22, Rue De St. Dines
53500 Ernie
France
Phone: 33-2-430-517-76
Fax: 33-2-430-569-10

INSTALLATION

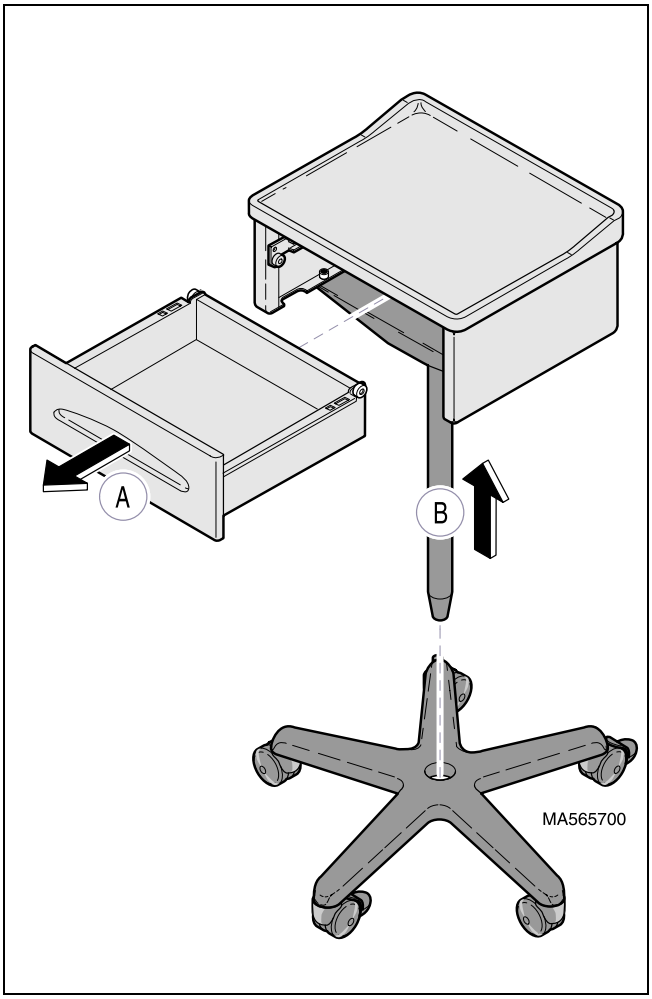

NOTE

Before working on ECG Cart remove all contents from top of cart and from drawer.

A. Remove drawer.

B. Separate caster base from pedestal by pulling upward.

NOTE

Lay unit on its top on a soft surface (to prevent scratching) for easier access when installing shelf.

© Midmark Corporation - 2001

INSTALLATION

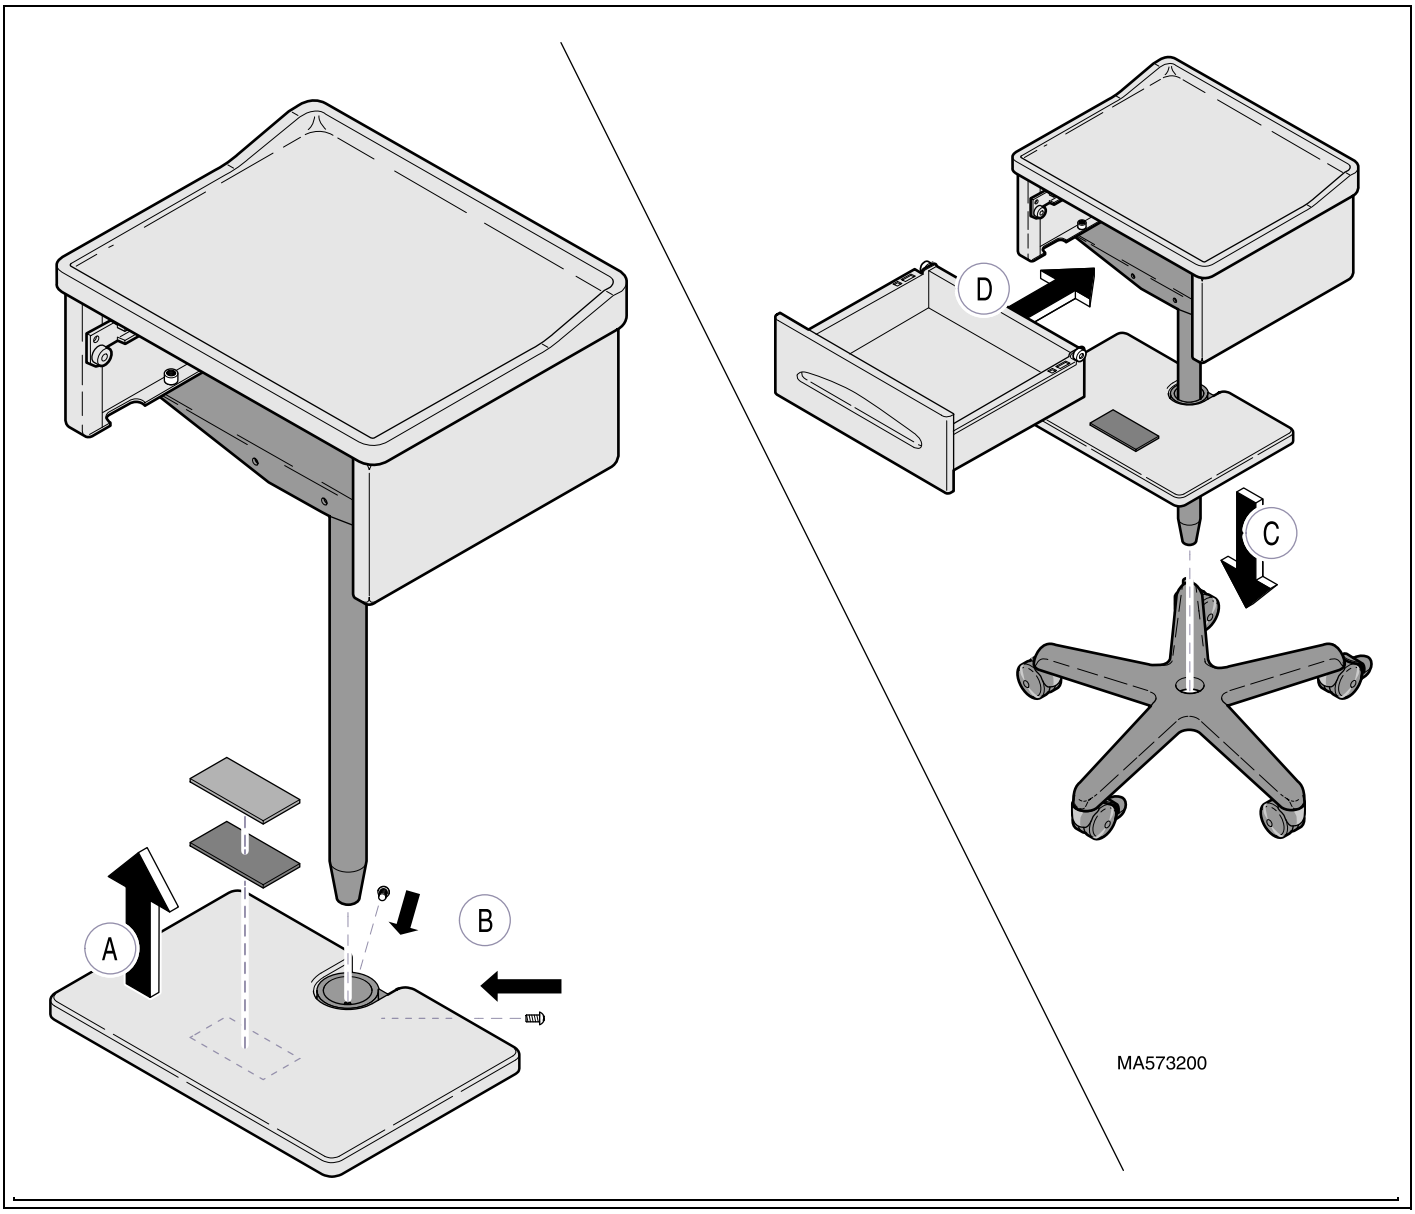

NOTE

Measure height of ECG printer that is to be located on shelf.

- **A.** Position shelf assembly onto cart post (as shown) so there is adequate clearance for ECG printer.
- **B.** Securely tighten the two phillips head screws to lock shelf in position.
- **C.** Insert pedestal into caster base, pressing firmly downward.
- **D.** Install drawer.

EQUIPMENT ALERT

Adhesive backed Velcro is supplied to secure printer to shelf. Position one piece onto bottom of printer and the other piece on shelf directly in line with printer velcro. Failure to secure printer could result in printer falling from shelf during transport, damaging printer.

© Midmark Corporation - 2001

MIDMARK®
Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542